



iCS-digital™ PSC test report

CONTACT PERSON		
Name: Julia Vullings	Phone: +3150098386	E-mail: stemcelltechnologycentergenetica.gen@radboudumc.nl
INSTITUTION / COMPANY		
Name: Radboudumc Stem cell technology center		
Address: Geert Grooteplein 10 6525GA Nijmegen		

PURCHASE ORDER (DATE)	REMAINING TEST
QUOT220404-1 (04/04/2022)	0


TEST DATE	CONTROL VALIDATION
April 07, 2022	Normal DNA control for the 24 probes: Passed

SUMMARY OF THE DETECTED COPY NUMBER VARIATIONS					
Sample	Passage	dsDNA (ng/μL)	dsDNA quantity	CNVs	Sex*
SCTC5	6	17	Good	Not detected	F


The results of this test are for research use only.

* If unknown, sex is deducted from the ChrX copy number; note that one ChrX can be detected in female cells that lost one ChrX, and two ChrX in male cells that gained one copy.

Copy number values:



SUMMARY OF THE DETECTED COPY NUMBER VARIATIONS																								
CHROMOSOME	1p	1q	2q	3p	4q	5q	6q	7p	7q	8q	9q	11p	12p	13q	14q	15q	16q	17p	17q	18q	19p	20q	22q	Xp
SCTC5																								

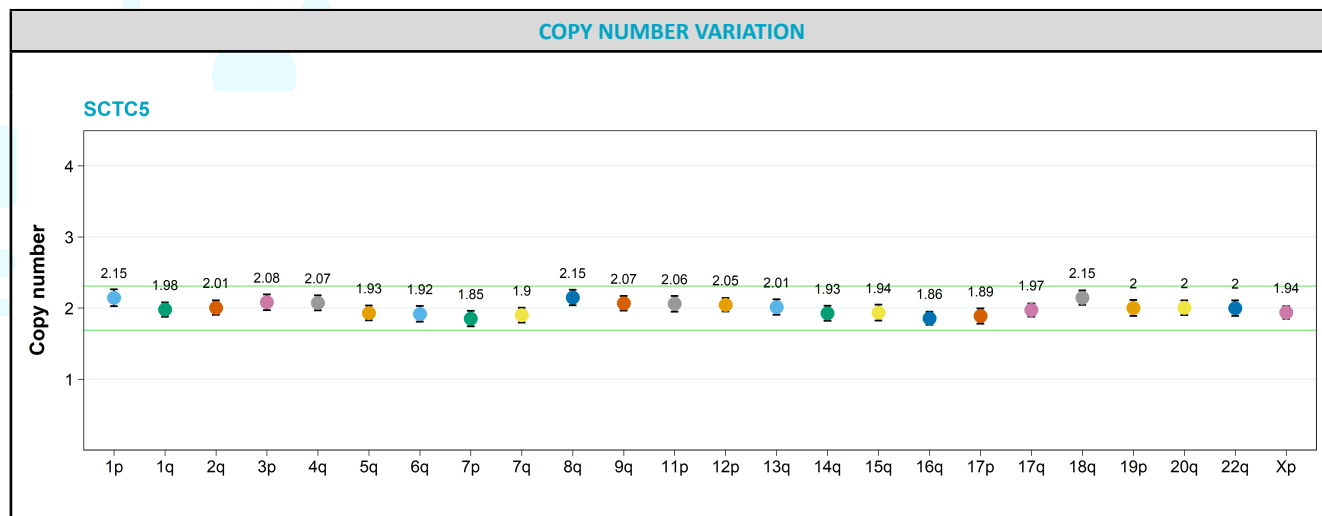


Elena Hauser
Platform Manager