


Cell line name	BIHi292
Bank / clone ID	Clone 2
Passage No.	14
Date of testing	26.07.2023
Protocol	8.4. Testing for remaining Sendai virus_CytoTune 2.0

Results

2 % standard agarose gel with DNA stain Ethidiumbromid 7µL/400 mL

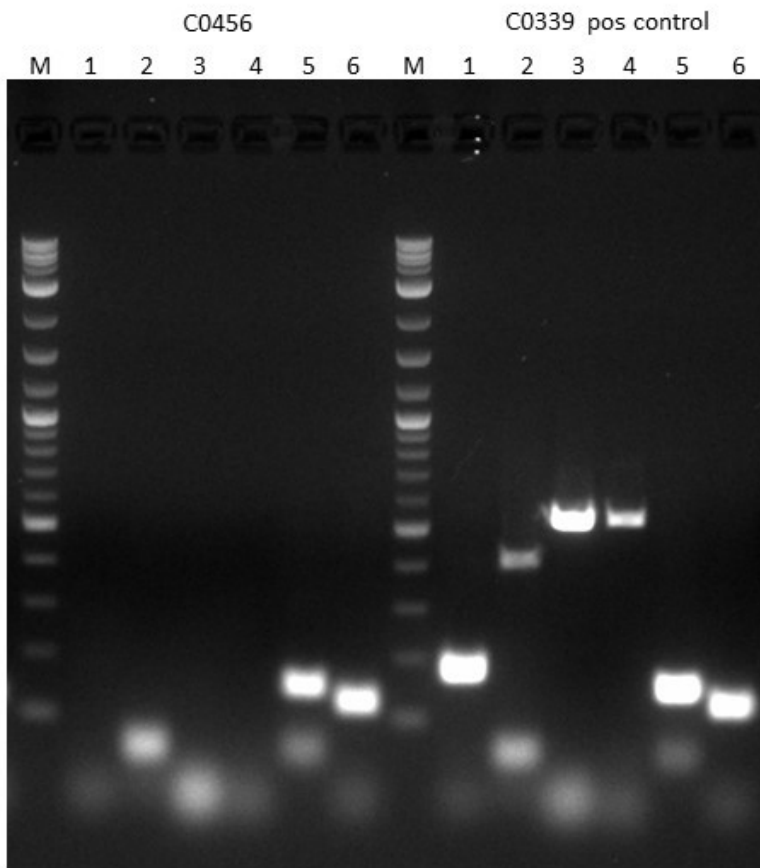

cDNAs

cDNA sample	Clone name / passage
C0456	BIHi292-cl.4 p14
C0339	SenV pos ctr.

Primer

	Primer	Size
1	SeV OL0109/10	181 bp
2	SeV_Klf 4 OL0111/2	410 bp
3	SeV_cMyc OL0113/4	532 bp
4	SeV_KOS OL0115/6	528 bp
5	Hu18sRNA OL0107/8	152 bp
6	beta-Actin OL0312/13	128 bp

PCR Results - Conclusion

The cell line is tested negative for Sendai virus.

Date 27.07.2023