



Certificate of analysis

SFC121-03-02

Operator: Jane Vowles

Date: 17/02/2016

Supervisor: Sally Cowley

Date: 19/08/2016

Signature:

SACowley


Source of fibroblasts and reprogramming information

- SF121 from Oxford University 02/04/2014
- Reprogrammed at UOXF-S
- Reprogrammed on 28/08/2015 at passage 3, JV
- Cytotune v2 WP3 SOP10


Viability post-thaw and Morphology according to SOP19 passage 10

- Cell count immediately post-thaw 2.9×10^6
- Viability immediately post-thaw 90%
- Photo at 24h and 3 day post-thaw (scale bar = $100\mu\text{m}$):

24h post-thaw 80% plated

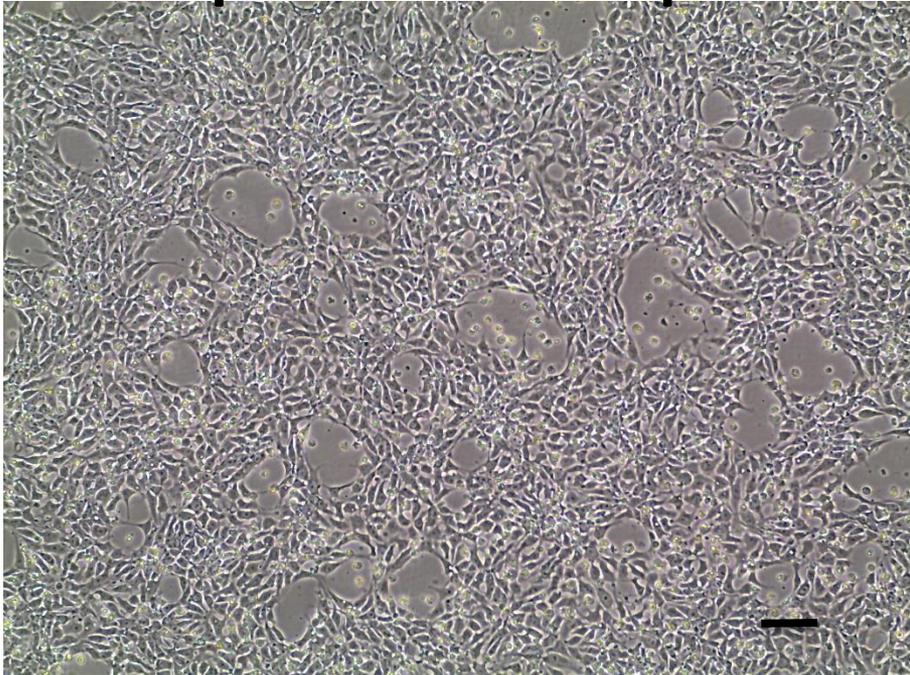


Day 3 post-thaw 20% plated

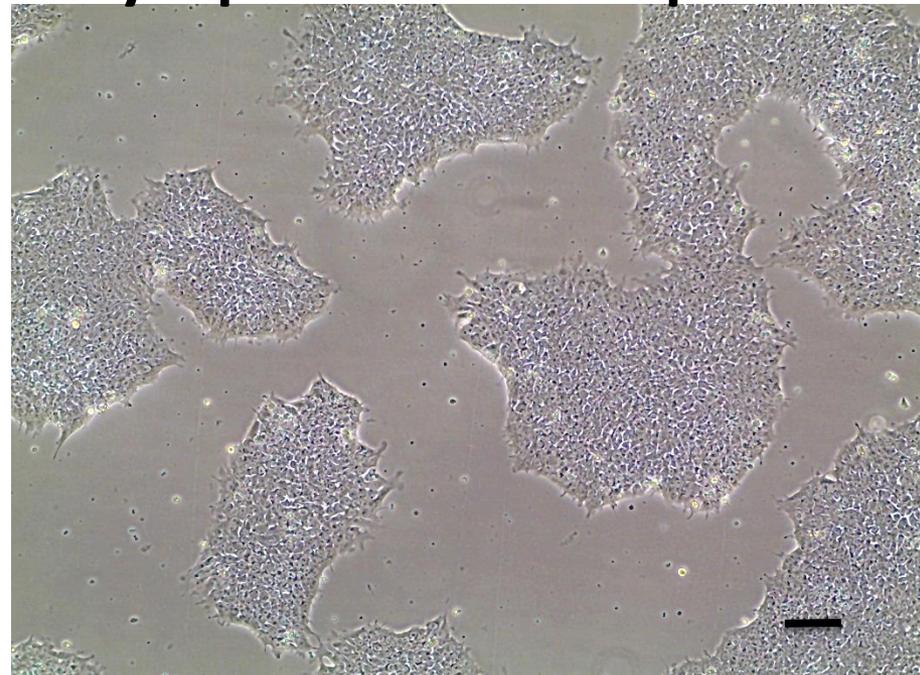

Sendai clearance: according to WP3 SOP15 undetectable at passage 10

2Log ladder
Sendai virus
KOS
Klf4
C-Myc
Actin

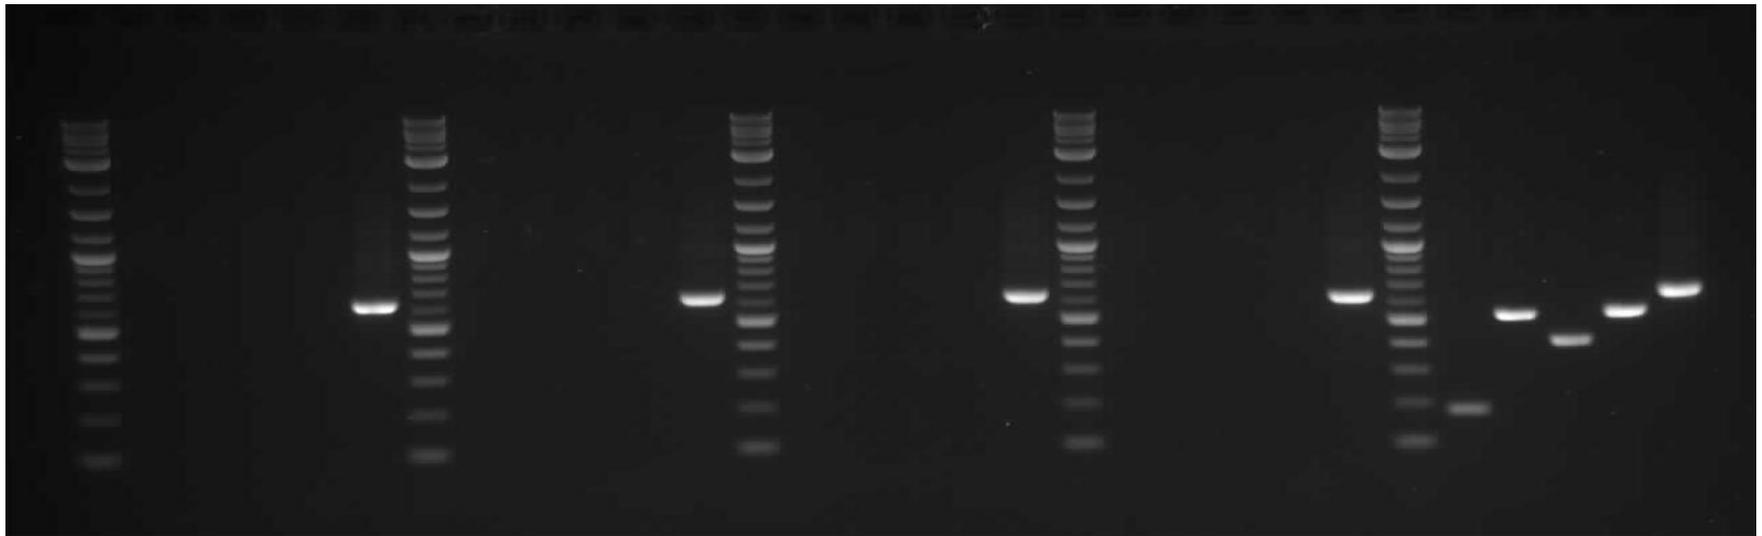

SFC121-03-02

SFC867-04-09

SFC867-04-12

- control

+ control

Product sizes: SeV 181bp; KOS 528bp; SeV-Klf 410bp; SeV-Myc 532bp; Actin 623bp

Mycoplasma Test:

According to MycoAlert Lonza LT07-318 undetectable at passage 10

Sample	Clone	Passage number	Initial	Reading 1	Reading 2	Ratio/Status
+ve control				2.99	167.90	56.15
-ve control				3.36	0.43	0.13
13	SFC121-03-02	p10	JV	2.50	1.37	0.55

Results mean


Ratio **0 - 0.999** negative for mycoplasma

Ratio **1 – 1.3** Borderline Result (retest required)


Ratio above **1.3** positive for mycoplasma

Flow cytometric analysis according to WP3 SOP 20 and 21 passage 17

Tra-1-60:

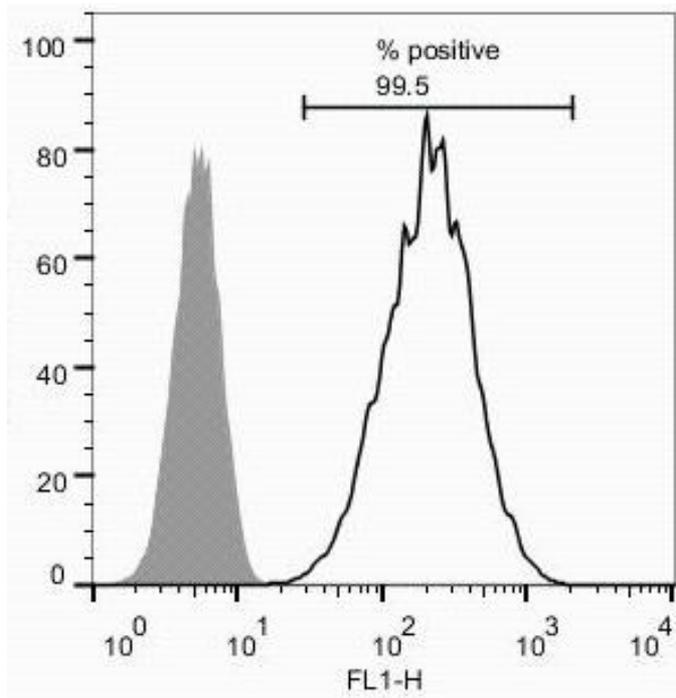

NANOG:

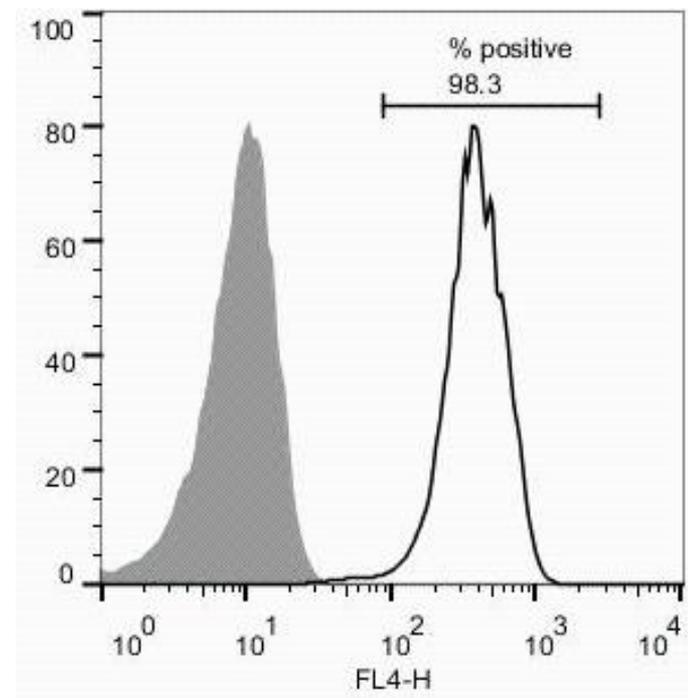

SNP analysis

according to WP3 SOP Preparation of DNA and RNA samples for Illumina arrays

- Passage 10
- Identity to parent fibroblasts confirmed
- Karyotype abnormalities: none detected
- For details and raw data see StemDB