



Certificate of analysis

SFC856-03-08

Operator: Galbha Duggal

Date: 13/08/2015

Supervisor: Zam Cader

Date: 12/02/2016



Signature: *Zam Cader*

Source of fibroblasts and reprogramming information

- SF856 from Oxford University Hospitals, 07/05/2014
- Reprogrammed at UOXF WIMM
- Reprogrammed on 09/10/14 at passage 4
- Cytotune v2 WP3 SOP10


Viability post-thaw and Morphology according to SOP19 passage 20

- Cell count immediately post-thaw 1.96×10^6
- Viability immediately post-thaw 91%
- Photo at 24h & day 4 post-thaw (scale bar = $100\mu\text{m}$):

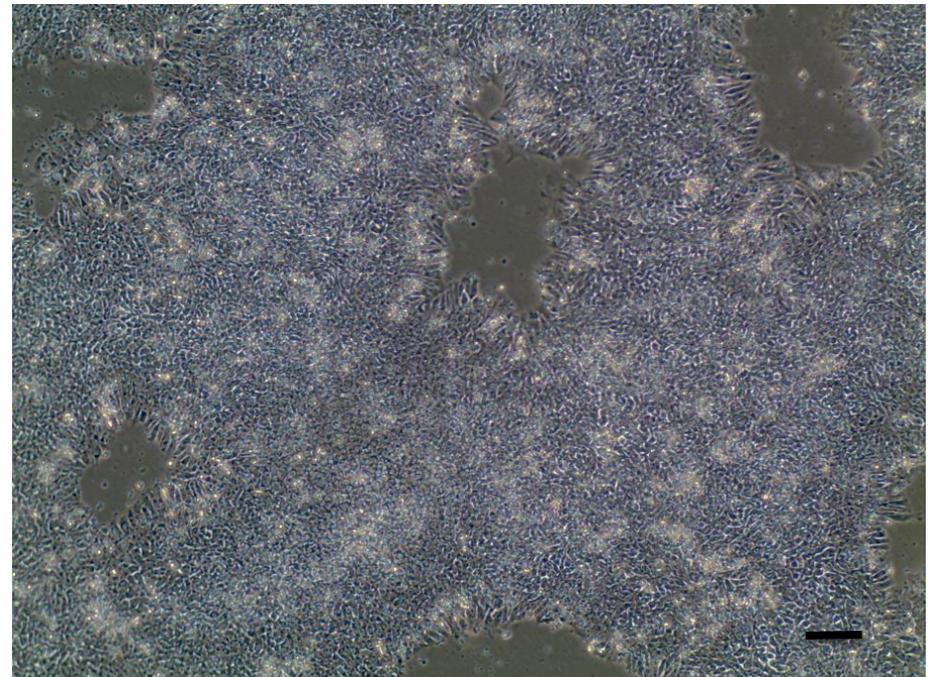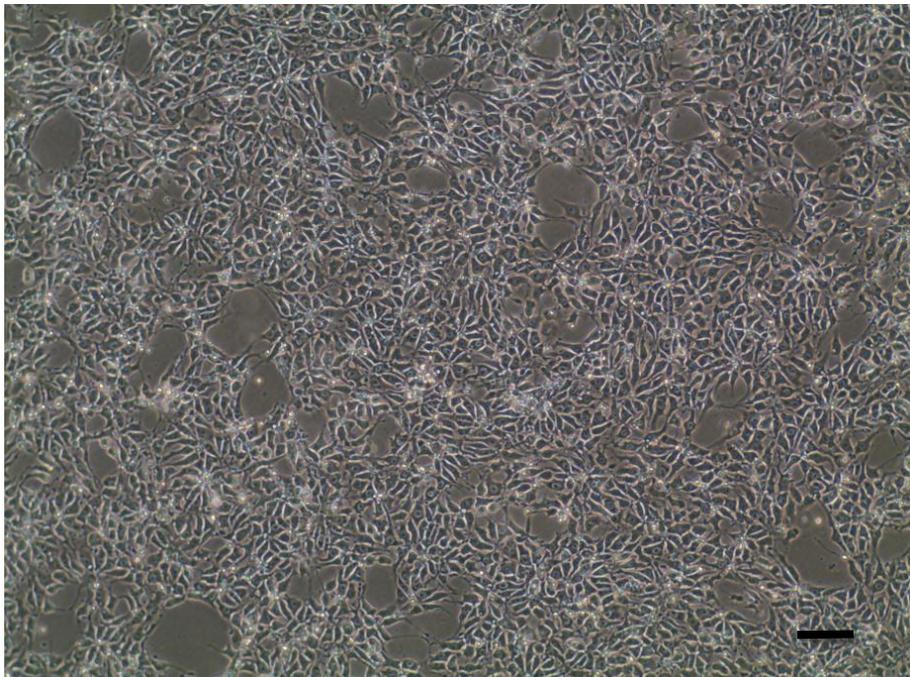

Sendai clearance: according to WP3 SOP15 undetectable at passage 20

100bp ladder
Actin
Sendai Virus
KOS
C-Myc
Klf4
100bp ladder
Actin
Sendai Virus
KOS
C-Myc
Klf4

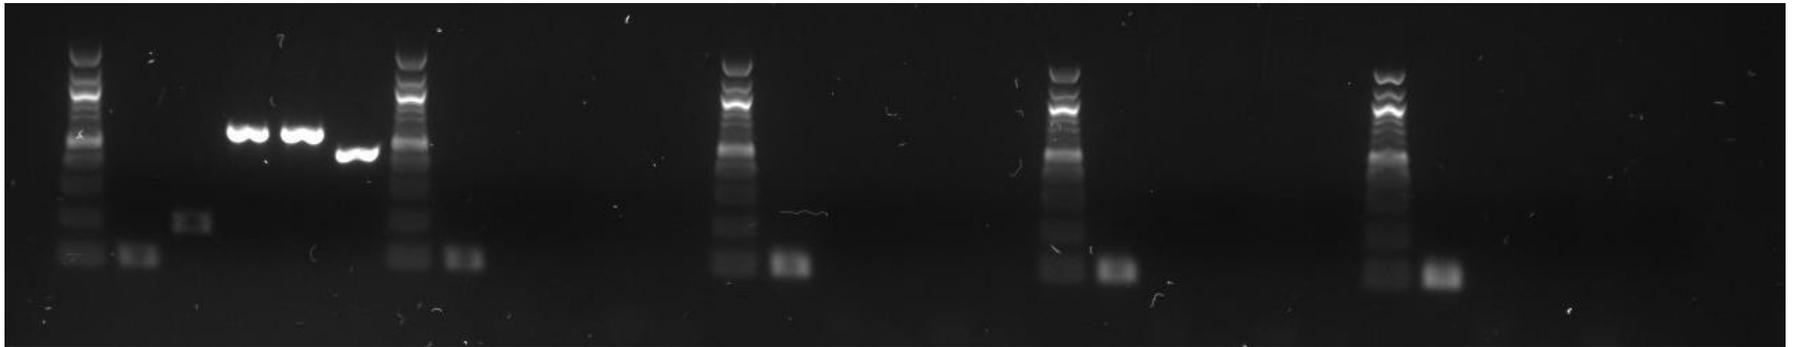

+ control

SFC180-01-01

SFC856-03-07

SFC856-03-08

SFC856-03-04

Product sizes: Actin 92bp; SeV 181bp; SeV KOS 528bp; SeV-Myc 532bp; SeV-Klf 410bp;

Mycoplasma Test:

According to MycoAlert Lonza LT07-318 undetectable at passage 20

Sample	Passage Number	Initials	Reading 1	Reading 2	Ratio/Status
+ ve control			54	5829	107.94
- ve control			105	77	0.73
SFC856-03-08	p20	GD	37	26	0.70

Results:


Ratio **0 - 0.999** negative for mycoplasma

Ratio **1 – 1.3** Borderline Result (retest required)


Ratio above **1.3** positive for mycoplasma

Flow cytometric analysis according to WP3 SOP 20 and 21 passage 20

Tra-1-60:

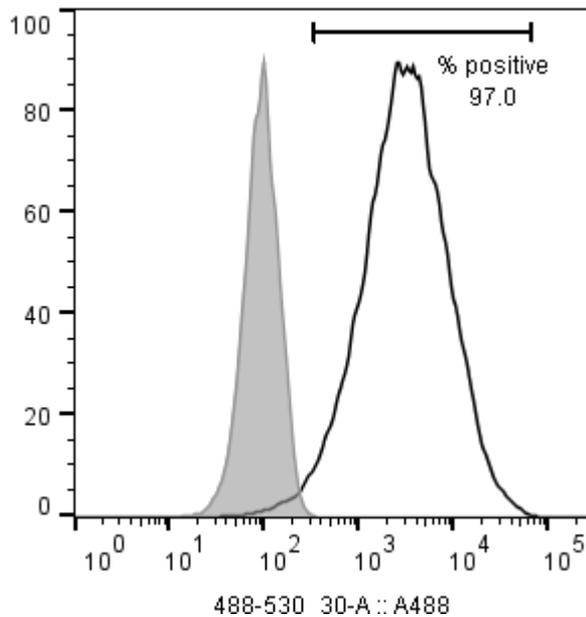

NANOG:

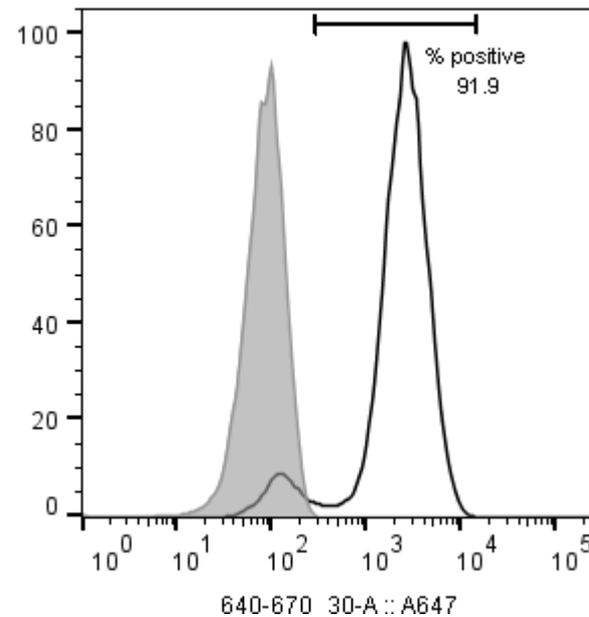

SNP analysis

according to WP3 SOP Preparation of DNA
and RNA samples for Illumina arrays

- Passage 20
- Identity to parent fibroblasts confirmed
- Karyotype abnormalities: none detected
- For details and raw data see StemDB